

DATE February 19, 1964

SHEET 1 OF 2

TMC SPECIFICATION NO. S-818

COMPILED


CHECKED

TITLE: Test Procedures TMA 10K

APPROVED

I. Equipment Required:

- A. Variac
- B. Transformer, TF-201, or Equivalent.
- C. 5 AMP. Calibrated Standard RF ammeter.

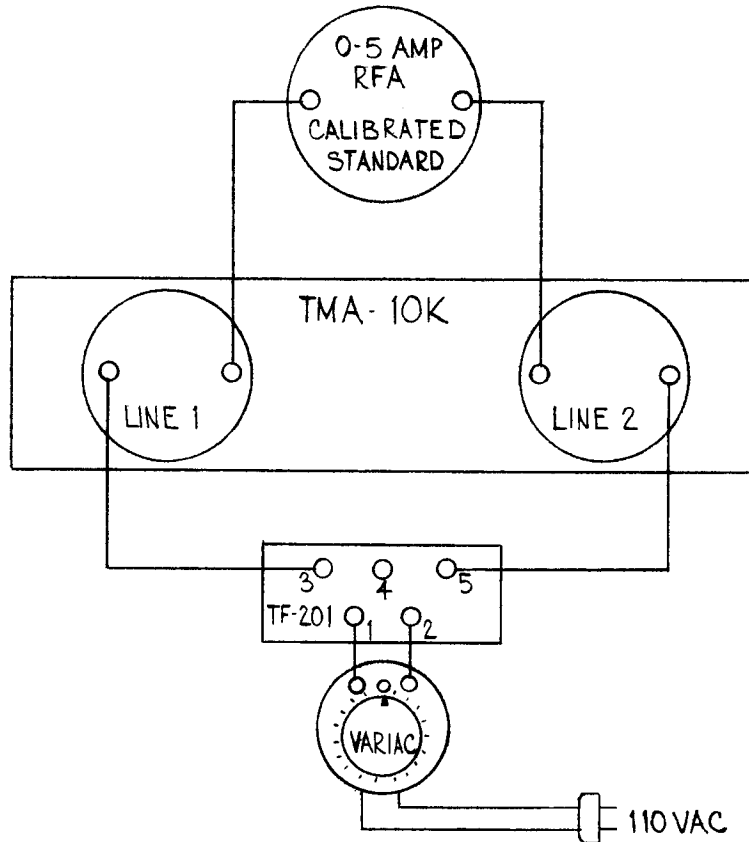

- II. Procedure: Check meters for Zero adjust and before plugging into 110 VAC outlet, set variac to ZERO. By adjusting the variac for a 3 amp and 5 amp deflection on the calibrated standard, the Line 1 and Line 2 meters, when compared with the calibrated standard, should read within 5% of the full scale value. Record Line 1 and Line 2 meter readings on test data sheet.

DATE February 19, 1964
SHEET 2 OF 2

TMC SPECIFICATION NO. S-818

E
COMPILED

JZ
CHECKED

TITLE: Test Procedures TMA 10K

DB
APPROVED

TMA-10K

TEST DATA SHEET

CALIBRATED METER
STANDARD

LINE #1
METER

LINE #2
METER

3 RFA

 RFA

 RFA

5 RFA

 RFA

 RFA

Requirement:

Line 1 and 2 meter readings when compared to the Calibrated Meter Standard shall be within 5% of full value when checked at 60 cycles.

Manufacturing Number

Tested By

Approved By

Date
